


# INTENTION HEALTH RESEARCH STUDY TO TEST THE EFFECTIVENESS OF BIOPROTEC CHIPS ON THE STRESS RESPONSE TRIGGERED BY EMF EMISSIONS

## Testing Equipment Biomeridian MSA-21 Professional Device (FDA Registered)

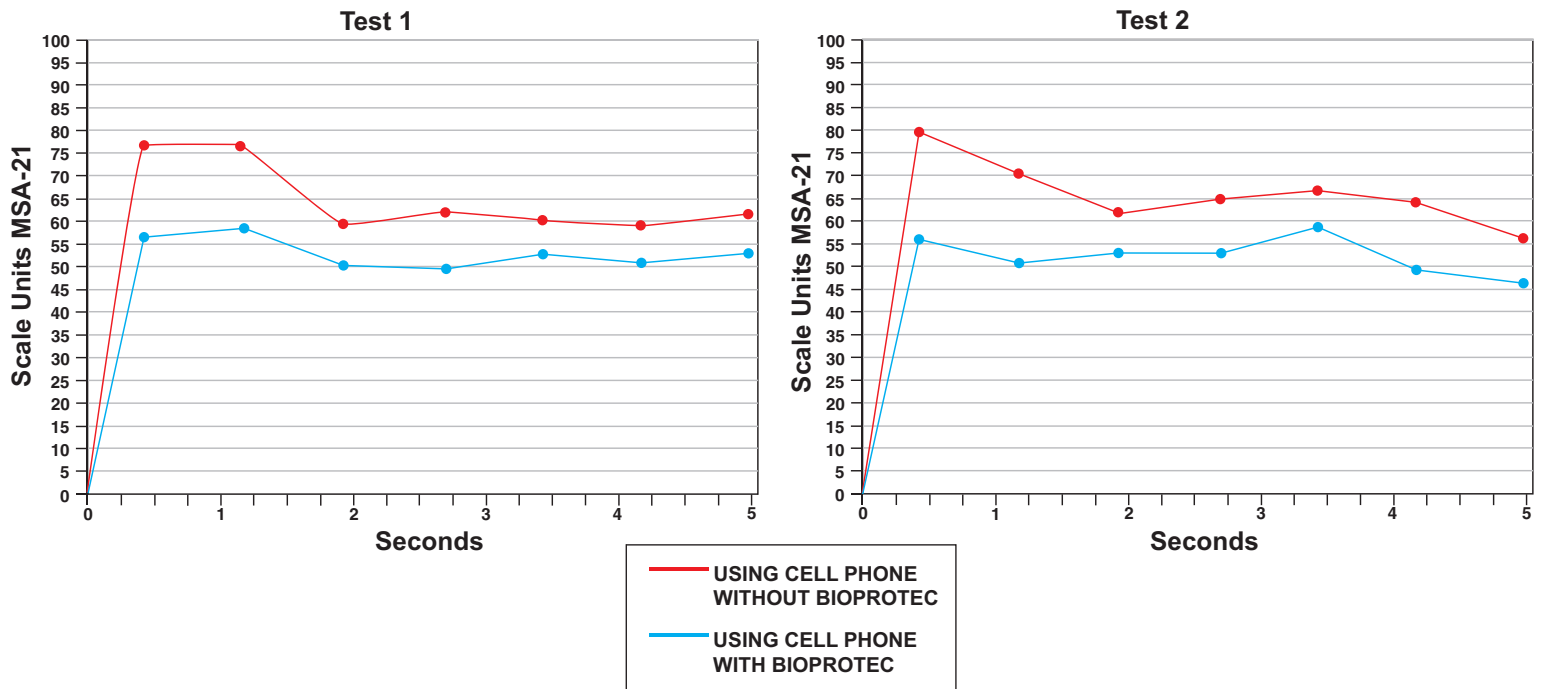

Many functional or energy medical devices, such as the BioMeridian MSA-21 Professional testing device used in this study are assessed on the research of Dr. Reinhold Voll. Voll established that there is a network of energy channels, called meridians, flowing through the body. Meridian points, some of which correlate to acupuncture points, can be used to collect energetic data. Dr. Voll demonstrated that the body's organs are associated with different energy meridians. Imbalances in various organs are believed to manifest themselves as energetic disturbances in the associated meridians. These energetic meridians are also highly responsive to external stressors, almost immediately.

These points represent the condition of the entire human energy system and, within seconds, reflect physical reactions to the exposure of EMF. Also, the body's compensatory reactions through homeostasis can immediately be measured and evaluated through these points. The MSA-21 Professional by Biomeridian (an FDA registered device) was used as the measuring device. It is a computerized stress assessment system that measures stress in up to 60 different parts of the human body. It is currently used by over 1500 physicians in both the U.S. and many other countries as an important indicator of resistance to stress in essential bio-systems throughout the body.

For purposes of speed and understanding we analyzed the body in seven key areas: 1-LYMPHATIC, 2-LUNG, 3-LARGE INTESTINE, 4-NERVOUS SYSTEM, 5-CIRCULATORY SYSTEM, 6-ALLERGY, 7-CELLULAR METABOLISM.

In each of these areas, the individual was measured on a data output scale of 0-100. The ideal target zone falls within the 45-55 scale unit range. Doctors say that with MSA-21 System, any measurement above 55 is stressful as it indicates excess energy, or an inflamed condition in that part of the human biofield. Any measurement below 45 is also stressful, because a lower number represents impaired, weakened, or blocked energy systems. The closer the measurements are to 50, the closer they are to actually being in a state of homeostasis. Average test measurements took approximately 4-6 minutes so as to negate the element of time compensation.

In summary under the influence of the BIOPROTEC chip the disturbance of the body's stress response when subjected to EMF exposure is harmonized or dampened back to a healthy standard range. This in fact demonstrates the positive effect of these devices.